Publication No. 7C8287
28JAN98

HEALTH IMAGING

DIAGRAMS
for the
Kodak X-Omat 3000 RA INTEGRATED PROCESSOR
in a *Kodak X-Omat* MULTILOADER 300 PLUS

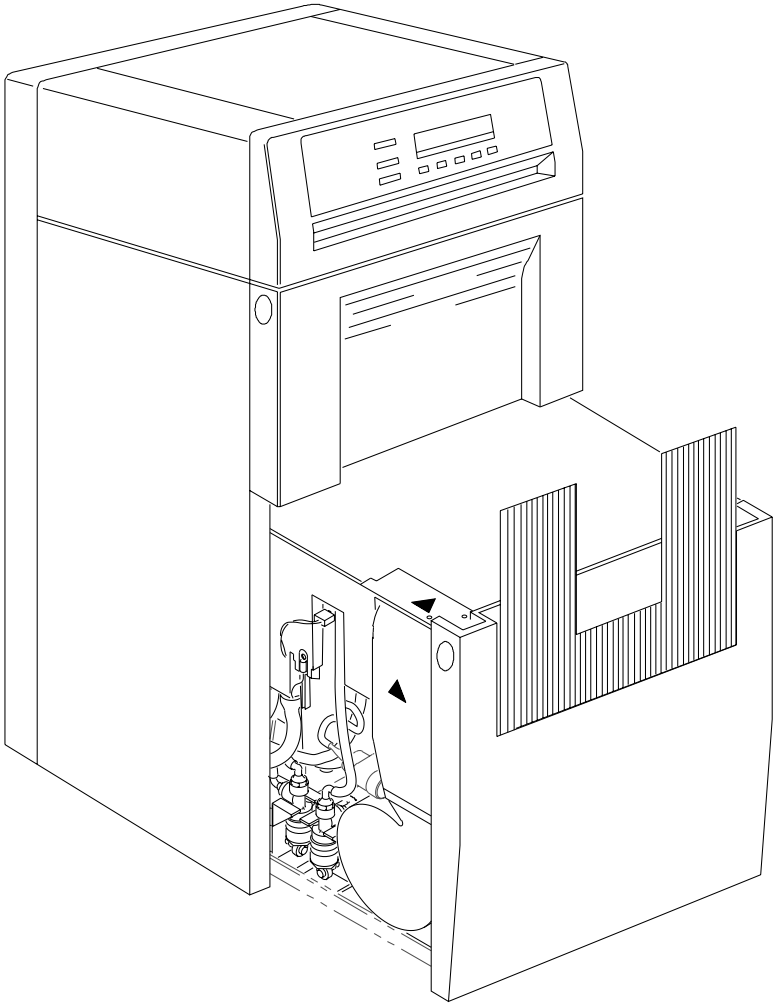

© Eastman Kodak Company, 1999

PLEASE NOTE The information contained herein is based on the experience and knowledge relating to the subject matter gained by Eastman Kodak Company prior to publication.

No patent license is granted by this information.

Eastman Kodak Company reserves the right to change this information without notice, and makes no warranty, express or implied, with respect to this information. Kodak shall not be liable for any loss or damage, including consequential or special damages, resulting from any use of this information, even if loss or damage is caused by Kodak's negligence or other fault.

This equipment includes parts and assemblies sensitive to damage from electrostatic discharge. Use caution to prevent damage during all service procedures.

Table of Contents

Description	Page
EXTERNAL WIRING DIAGRAM	3
ELECTRICAL BOX	4
AC CIRCUIT DIAGRAM	5
DC CIRCUIT DIAGRAM	6

Figure 1 **EXTERNAL WIRING DIAGRAM**

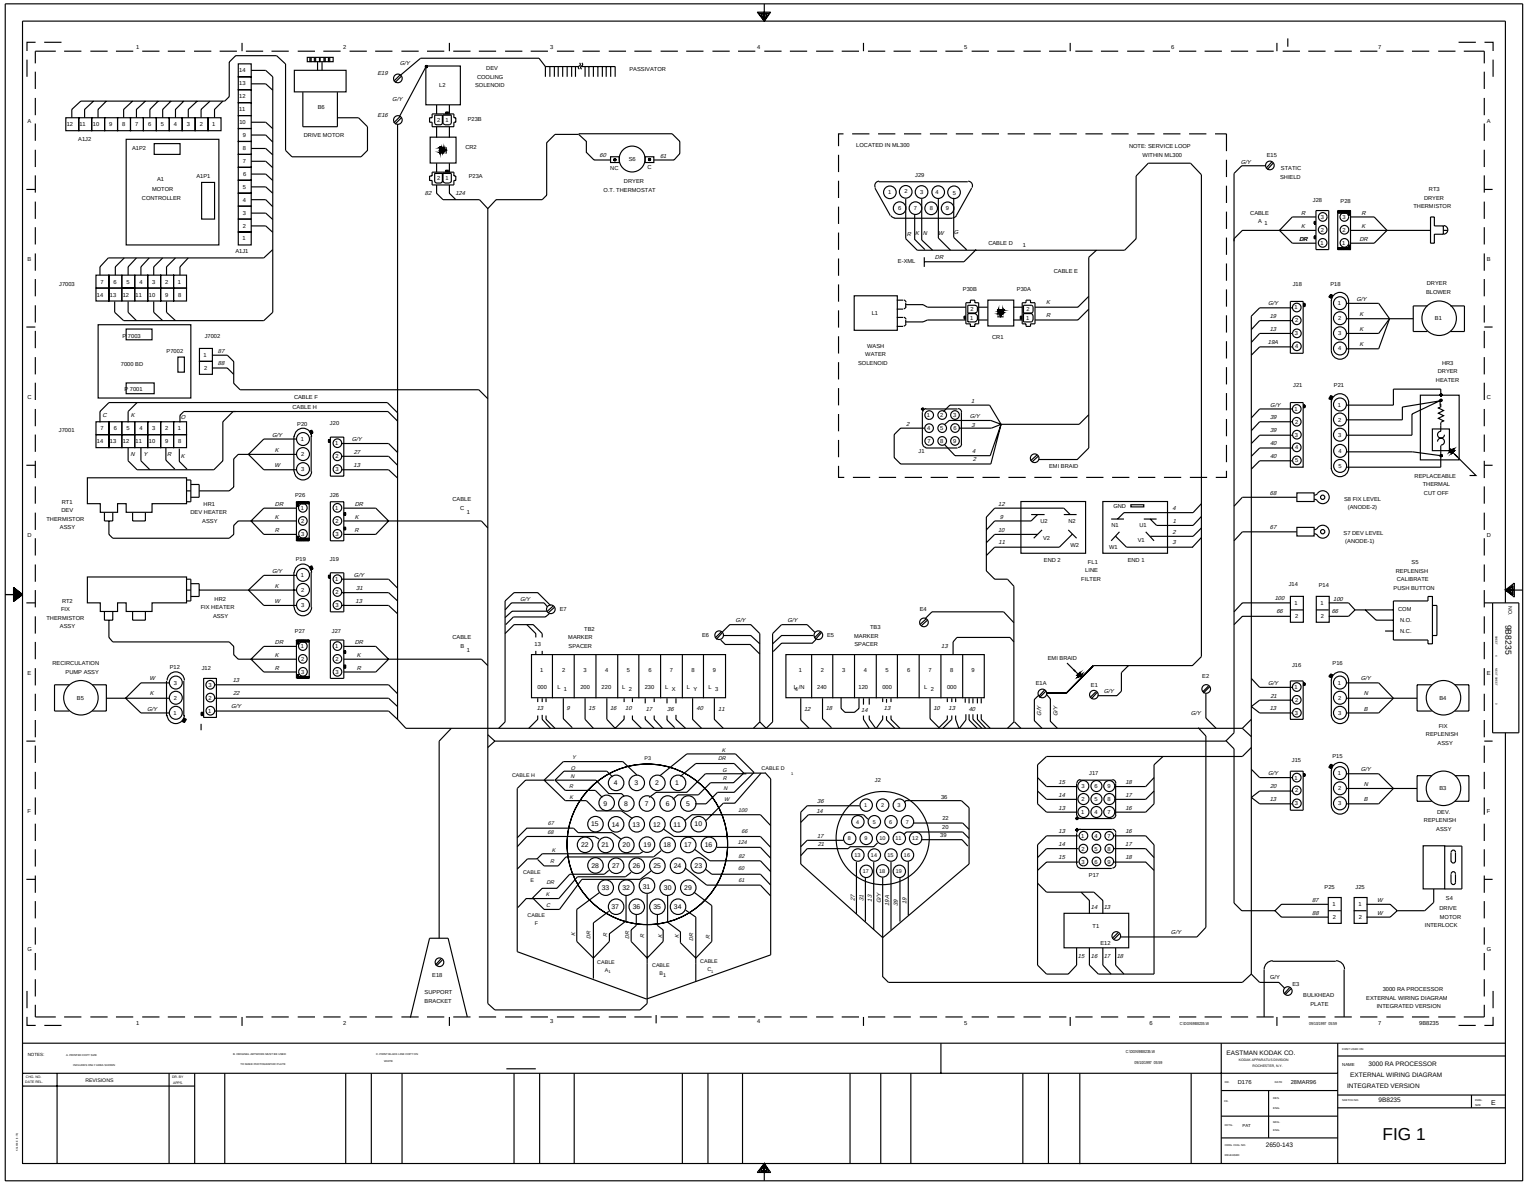

H166_0001FC

Figure 2 **ELECTRICAL BOX**

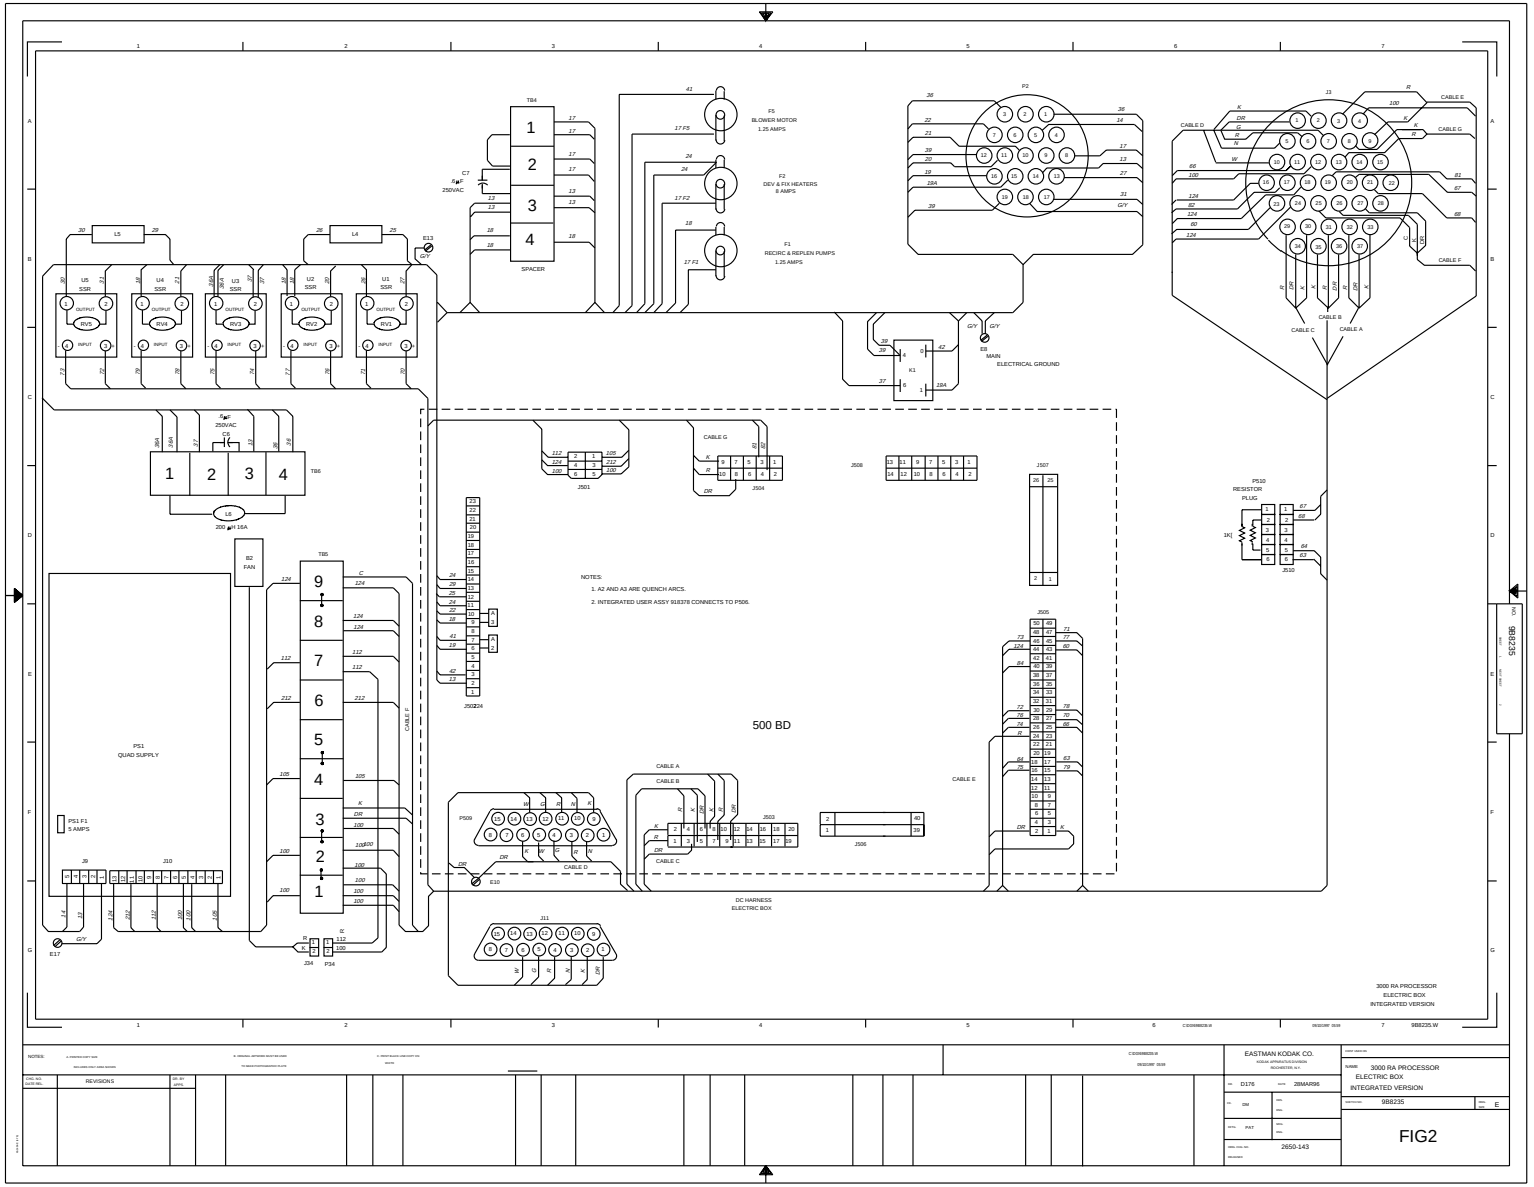

H166_0002FC

Figure 3 **AC CIRCUIT DIAGRAM**

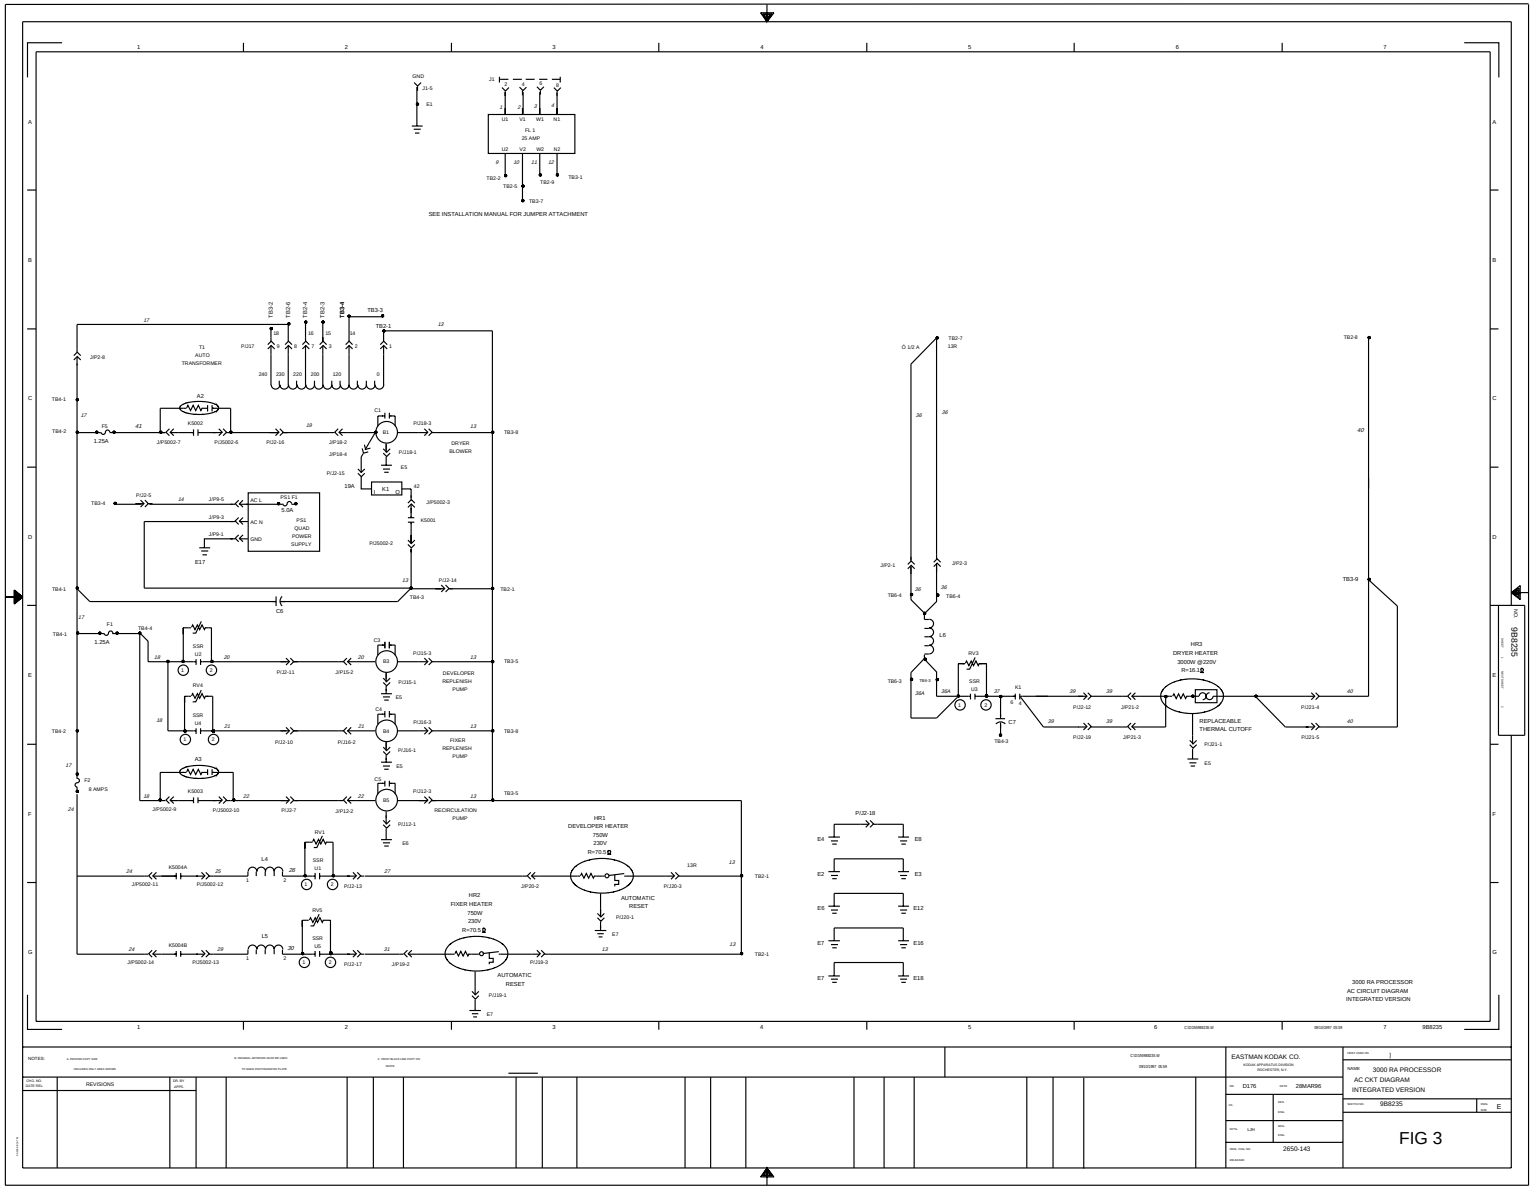

H166_0003FC

Figure 4 **DC CIRCUIT DIAGRAM**

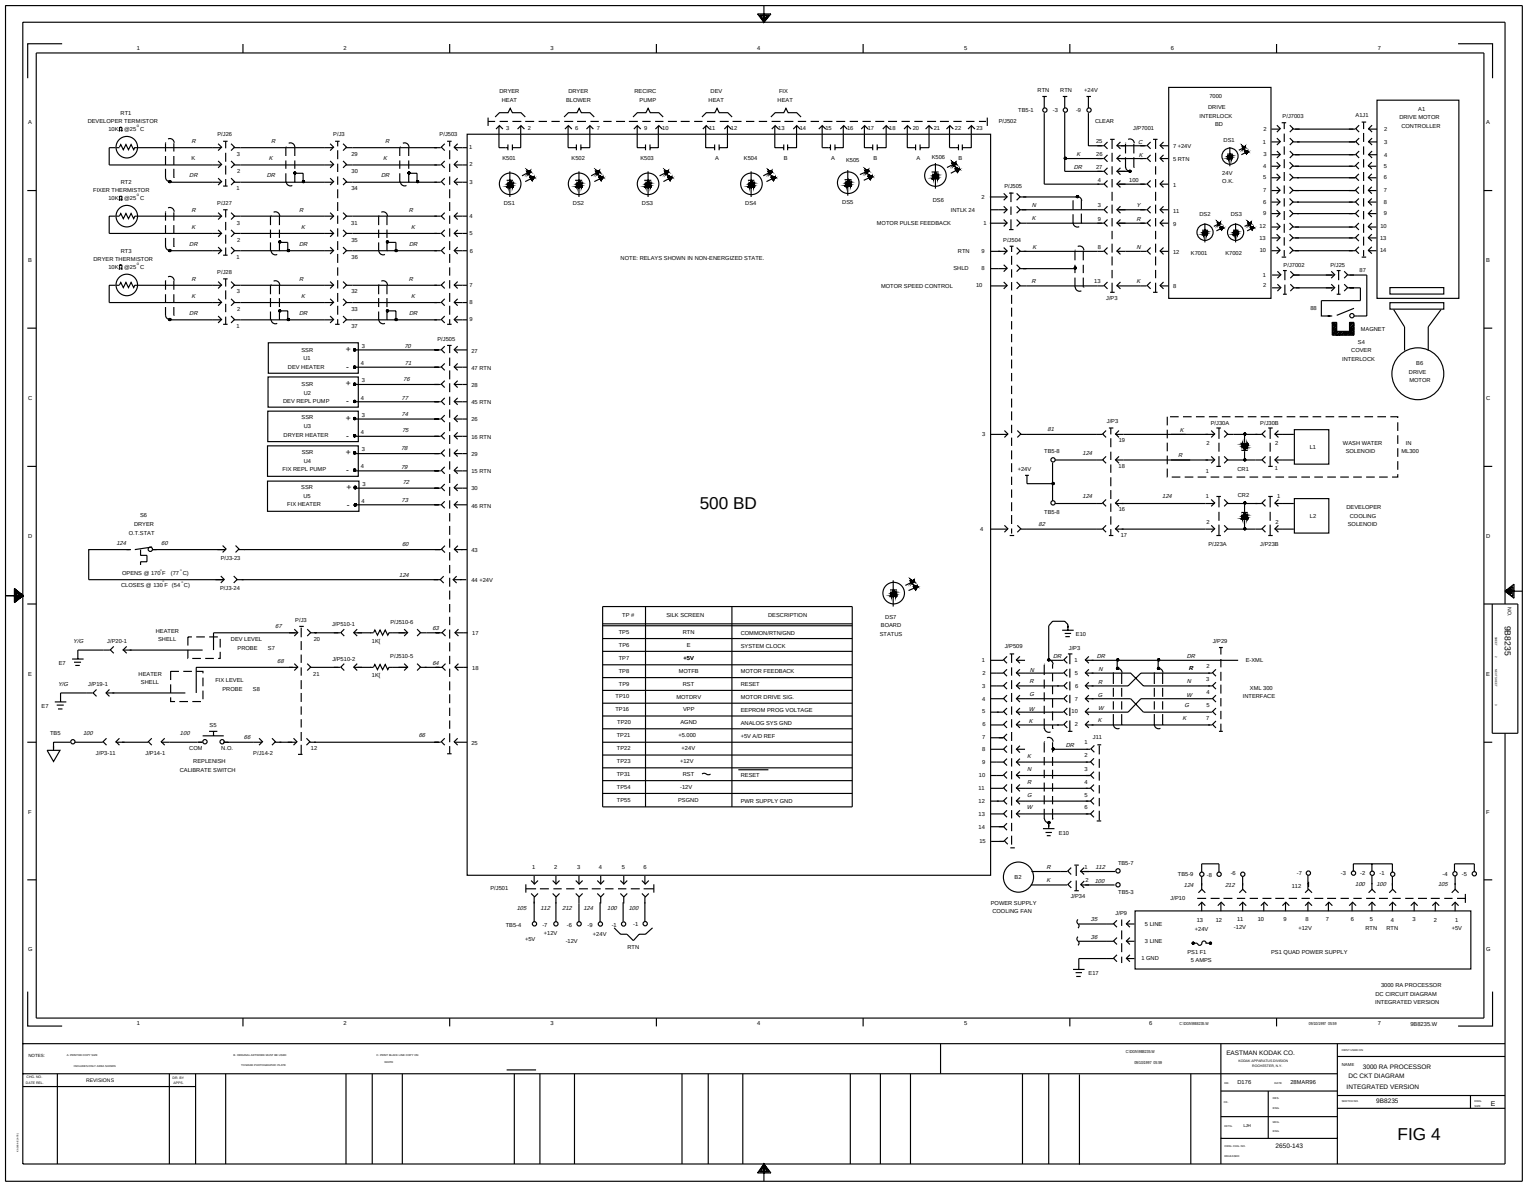

TP #	SILK SCREEN	DESCRIPTION
TP5	RTN	COMMON/RTN/GND
TP6	E	SYSTEM CLOCK
TP7	+5V	
TP8	MOTFB	MOTOR FEEDBACK
TP9	RST	RESET
TP10	MOTDRV	MOTOR DRIVE SIG.
TP16	VPP	EEPROM PROG VOLTAGE
TP20	AGND	ANALOG SYS GND
TP21	+5.000	+5V A/D REF
TP22	+24V	
TP23	+12V	
TP31	RST ~	RESET
TP54	-12V	
TP55	PSGND	PWR SUPPLY GND

H166_0004FC

Table 1 Publication History

Print Date	Pub. No.	ECO No.	Affected Pages	File Name	Notes
January 1998	7C8287		All	di3488_1_28jan98	First Printing

Kodak and *X-Omat* are trademarks

Printed in U.S.A. • di3488_1.fm

EASTMAN KODAK COMPANY
Rochester, NY 14650

HEALTH IMAGING